

Characteristics of very slow stepping in healthy adults and validity of the activPAL3™ activity monitor in detecting these steps

Stansfield, Ben; Hajarnis, Mugdha; Sudarshan, Radhika

Published in:
Medical Engineering and Physics

DOI:
[10.1016/j.medengphy.2014.10.003](https://doi.org/10.1016/j.medengphy.2014.10.003)

Publication date:
2015

Document Version
Author accepted manuscript

[Link to publication in ResearchOnline](#)

Citation for published version (Harvard):
Stansfield, B, Hajarnis, M & Sudarshan, R 2015, 'Characteristics of very slow stepping in healthy adults and validity of the activPAL3™ activity monitor in detecting these steps', *Medical Engineering and Physics*, vol. 37, no. 1, pp. 42-47. <https://doi.org/10.1016/j.medengphy.2014.10.003>

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

If you believe that this document breaches copyright please view our takedown policy at <https://edshare.gcu.ac.uk/id/eprint/5179> for details of how to contact us.

1 **Title**

2 Characteristics of very slow stepping in healthy adults and validity of the activPAL3™ activity
3 monitor in detecting these steps

4

5 **Authors**

6 Ben Stansfield^a, Mugdha Hajarnis^a, Radhika Sudarshan^a.

7 ^aSchool of Health and Life Sciences, Glasgow Caledonian University, Glasgow, UK

8

9 **Corresponding author**

10 Ben Stansfield.

11 School of Health and Life Sciences, Glasgow Caledonian University, Cowcaddens Road, Glasgow, G4

12 OBA, UK. Tel: 00(44) 141 2731551. Email: ben.stansfield@gcu.ac.uk

13

14 **Conflict of Interest Statement**

15 Stansfield has received grant funding in the past from PAL Technologies Ltd (manufacturer of the
16 activPAL3 monitor) towards unrelated research work. Stansfield has received no personal payment
17 as part of the current study or for previous research work.

18 Hajarnis and Sudarshan have no conflict of interest to declare.

19

20

21

22 **Highlights**

23 The validity of the activPAL3™ activity monitor was assessed at low speed and cadence

24 A treadmill walking protocol was used from 1.0 down to 0.1m/s

25 Above 0.5m/s and 69 steps/min over 90% of steps were detected.

26 Below these thresholds performance reduced rapidly.

27 At 0.1m/s and below 27 steps/min no steps were detected.

28

29

30 **Title**

31 Characteristics of very slow stepping in healthy adults and validity of the activPAL3™ activity
32 monitor in detecting these steps

33 **Abstract**

34 The use of activity monitors to objectively measure stepping activity allows the characterisation of
35 free-living daily activity performance. However, they must be fully validated. The characteristics of
36 very slow stepping were examined and the validity of an activity monitor, the activPAL3™ (PAL
37 Technologies Ltd. Glasgow, UK) to detect these steps was assessed. 10M/10F healthy adults
38 (36±10y) performed a treadmill walking protocol from 1.0m/s down to 0.1m/s (0.1m/s increments)
39 whilst wearing AM under video observation (gold standard). Within the 800 stepping periods
40 recorded the proportion of steps correctly detected by the activPAL3™ was explored against speed
41 and cadence. Below 0.4m/s walking began to be intermittent, stepping interspersed with stationary
42 postures. At 0.1m/s almost 90% of walking periods were intermittent. The percentage of steps
43 detected was over 90% for walking speed at or above 0.5m/s and cadence at or above 69 steps/min.
44 However, below these limits % steps detected reduced rapidly with zero steps detected at 0.1m/s
45 and at or below 24 steps/min. When examining the stepping activity of groups with limited stepping
46 cadence the above thresholds of performance should be considered to ensure that outcomes are
47 not misinterpreted and important very slow stepping activity missed.

48

49 **Keywords**

50 Gait speed; cadence; step length; validity; activPAL3 activity monitor.

51

52 Main text word count: 3986

53 **Introduction**

54 Physical activity performance is essential for the maintenance of good health with international
55 guidelines recommending the performance of minimum volumes of physical activity [1]. Stepping is
56 one of the key activities that can be used to fulfil the physical activity recommendations. It has been
57 estimated that 7,000 steps per day are associated with the development and maintenance of
58 musculoskeletal, cardiorespiratory and neuromotor fitness [2]. Engagement in stepping activity is
59 also required to facilitate the performance of every-day activities around the home and into the
60 wider community. Therefore, it is of interest to be able to quantify the volume of stepping activity
61 that individuals perform in a free-living context, both to gauge the health benefits accrued and to
62 characterise daily living activity.

63 Stepping is performed at a range of different stepping rates (cadences) which equate to a range of
64 different translational speeds. Usual purposeful 'healthy' self-selected walking speed has been
65 observed to occur at approximately 1.3m/s (e.g. men 20-30y, 1.39m/s, women 70-80y, 1.27m/s [3]).
66 However, slower stepping activity is performed both in healthy populations and in populations with
67 pathology affecting walking speed. In their review of the literature Peel et al [4] report gait speeds
68 as low as 0.11m/s in geriatric populations. Studenski et al [5] reviewed evidence of the relationship
69 between self-selected gait speed and survival, providing information relating to speeds down to
70 0.2m/s to fully characterise life course outcomes. It is possible that relatively slow stepping activity
71 forms a considerable proportion of daily activity for sections of the population who do not regularly
72 perform purposeful walking out of the home (e.g. those with limited cardiorespiratory function). If
73 stepping activity is to be accurately objectively measured the full range of stepping rates used should
74 be characterised. Therefore, if the purpose of a device is to measure stepping activity it is important
75 that it is able to adequately detect stepping at slow stepping rates.

76 Accelerometer based devices are able to monitor stepping activity through analysis of the signal
77 resulting from movement of the wearer. An example, the PAL Technologies Ltd. family of monitors

78 (activPAL™ (uniaxial) and activPAL3™ (tri-axial), PAL Technologies Ltd, Glasgow, UK), use proprietary
79 analysis algorithms to determine stepping performance. Output from these monitors is in the form
80 of individual strides with allocated durations. This allows the calculation of instantaneous cadence
81 or true cadence [6]. The assessment of the activPAL™ monitor's performance has been carried out
82 across a range of speeds. Typical outcomes of the lowest speeds tested in healthy populations are,
83 mean 9.9y, 0.88m/s, correlation with video observation: $r=0.88$ [7]; females mean 18.5y, 0.89m/s
84 stepping agreement 0.3 steps [LOA 3.9- -3.3] [8]; mean 23y, speed 0.89m/s, within 1 ± 9 steps out of
85 approx. 200 [9]; mean 28y, speed 0.6m/s, 1.7% error [10]; mean 34.5y, speed 0.9m/s, <0.94% error
86 in step count [11]; older adults mean 72y, speed 0.67m/s, <1% error [12]. According to the
87 outcomes of these studies the activPAL™ has excellent validity for step detection. However, there is
88 emerging evidence that the monitor does not detect all steps when walking below these speeds.
89 Taraldsen et al [13] indicate that in both a reference population (mean 46.3y) and people with stroke
90 (mean 75.2y) and inpatients (mean 84.0y) steps were under-detected below 0.47m/s. Kanoun [14]
91 presents provisional results indicating that at 0.45m/s, for a group mean 23.5y, the percentage error
92 in steps detected was 3.5% with a range of 0-30%. Lutzner et al [15] report outcomes of assessment
93 in young healthy adults (23.6 SD 4.4y) of step detection for a treadmill based protocol across a wide
94 range of walking speeds from very slow 0.1m/s to very fast 2.6m/s. They indicate for the standard
95 placement of the activPAL™ that there is considerable reduction in step detection below 0.7m/s,
96 with a mean of less than 50% of steps detected at 0.4m/s compared to manual step count.

97 Whilst the literature reports stepping activity as low as 0.11m/s [4] it is possible that the mode of
98 progression at this speed is discontinuous, i.e. one step is taken followed by a pause before the next
99 step. The mode of stepping is not usually described in the literature. Knowledge of the minimum
100 continuous speed for linear progression would provide information for interpreting very slow
101 cadence stepping as recorded by a monitor. Intermittent stepping may be recorded as very slow
102 continuous stepping, perhaps leading to misinterpretation of free-living activity patterns. Low
103 cadence outcomes have been reported in the literature for the activPAL™ (e.g. Dall et al [6] report

104 cadence as low as 20 steps/min). It is important to understand what this stepping activity
105 represents and if these are likely to be continuous stepping bouts or to be intermittent stepping
106 reported as continuous stepping activity.

107 Ideally the validity of the monitors would be established under free-living conditions. However, this
108 is extremely time-consuming as the recognised gold standard is manually counted steps, usually
109 from a video recording. Long periods of data monitoring are, therefore, difficult to perform. A
110 compromise is to use laboratory based data collection methods over short time periods. These can
111 either involve over-ground walking or treadmill based protocols. If the aim of a study is to
112 systematically analyse a range of speeds of walking this is difficult to achieve using over-ground
113 walking; participants can only be asked to walk 'normally' or 'faster' or 'slower' than normal.
114 Treadmill walking provides a compromised in that speed can be finely controlled [15].

115 The aims of the current study were twofold: First to establish the relationship between speed of
116 walking and cadence at slow stepping rates, including the determination of the slowest speeds of
117 continuous stepping and secondly to establish the validity of the activPAL3™ physical activity
118 monitor to detect stepping at these slow stepping rates.

119

120 **Methods**

121 Twenty (10M/10F) participants, between 18 and 60 years of age, were recruited from staff and
122 students of Glasgow Caledonian University. Informed consent was obtained from the participants
123 and ethical approval for the study was obtained from the Glasgow Caledonian University School of
124 Health and Life Sciences Ethics Committee. Participants did not have any known neurological
125 conditions, lower limb dysfunction, vascular dysfunction that might affect walking or injury to the
126 lower limb sustained within the preceding 6 weeks. Participants' gender, height, weight and age
127 were recorded.

128 The physical activity monitor, the activPAL3™ (PAL Technologies Ltd, Glasgow, UK) was used in this
129 study. Two monitors were used, one on each thigh. The monitors were attached using PALStickies™
130 (PAL Technologies Ltd, Glasgow, UK) on the mid-line of the thigh at the mid-point between the
131 anterior superior iliac spine and the superior border of the patella as measured in a supine position.
132 Participants wore their own clothing and shoes (not high heels). The activPAL3™ detects each
133 stride. The number of steps was calculated as strides multiplied by 2 for each of the monitors.
134 Version 7.1.18 of the activPAL3™ software was used for all data processing.

135 Once the activPAL3™s had been put in place the participant mounted the treadmill (Woodway,
136 Waukesha, USA, Model PPS 55med, accuracy ± 0.007 m/s across 0.1-1.0m/s settings) and the session
137 commenced. The protocol outlined in Table 1 was followed with four stepping cycles performed by
138 each participant. Each stepping cycle followed one of two protocols:

139 A (Descending cycle) = decreasing from 1.0 m/s to 0.10 m/s, in 0.1m/s decrements each 30 seconds
140 B (Ascending cycle) = increasing from 0.10m/s to 1.0m/s, in 0.1m/s increments each 30 seconds

141 Each participant completed 2xA and 2xB cycles with the order of cycles manipulated to ensure equal
142 numbers of participants completed AB and BA sequences before and after the mid-testing break.
143 The walking cycles were programmed to run automatically under the control of the treadmill.
144 Acceleration and deceleration was completed within the first 1-2s of transition between speeds
145 within each cycle. Each cycle took 5 mins giving an overall protocol time of approximately 25 mins.
146 The entire session was video recorded in High Definition.

147

148 Insert Table 1 here

149

150 Data analysis

151 Time synchronisation was achieved between the video record and the activity monitors by
152 identifying the first stride of walking commencing at 1.0m/s in the activPAL3™ record and the
153 corresponding time point in the video. This time synchronisation was used across the whole walking
154 sequence which was continuously recorded on video.

155 From the video the timing of the 20s of stepping activity at the middle of the 30s period was
156 selected, i.e. leaving a 10s gap between evaluation periods for sequential speeds. Within the
157 identified 20s periods all steps (either left or right foot initial contact with the ground) were counted
158 and agreed by two observers. The total number of steps observed on video within the 20s period
159 was used as the gold standard measure.

160 The activPAL3™ Event output file (individual stride occurrence recorded against time) was examined
161 to identify the number of strides recorded during the same 20s periods as determined from the
162 video analysis. A stride was allocated to a time period if its start time was either precisely at the
163 start of the time period or it was within the time period. The number of steps was determined as
164 the number of strides multiplied by 2. The proportion of steps detected was determined by
165 calculating:

166 $\% \text{ steps detected} = (\text{number of steps detected by the activPAL3}^{\text{TM}} / \text{video step count}) \times 100$

167 Observations from the video were made to classify walking as either continuous (always one leg
168 moving in relation to the treadmill belt) or intermittent (where both legs were stationary in relation
169 to the belt at some point during the time period). The proportion of walks performed in an
170 intermittent manner was determined within speed and cadence bands.

171 If walks were performed in an intermittent way, then the time of walking would not have been the
172 entire 20s period. This means that the calculated mean speed and mean cadence would not be the
173 same as the true speed and cadence of the walking activity within the time period. For the purposes

174 of this report the mean speed and mean cadence are used to represent the stepping activity within
175 each time period.

176 The mean cadence of walking was calculated from the video based step count within the known
177 time period of 20s. The mean step length was calculated based on the calculated mean cadence and
178 the treadmill speed.

179 The relationship between the percentage of steps detected and the stepping speed and cadence of
180 stepping was explored by examining the percentage of steps detected by the activPAL3™. For all
181 walks performed at each stepping speed the median and interquartile range of the % steps detected
182 were determined. Also for all those bouts of stepping performed at a certain cadence the median
183 and interquartile range of the % steps detected were calculated. This provided a profile of how the
184 % steps detected changed with speed of stepping and cadence of stepping.

185 To take account of any effects due to synchronisation error or discrepancy in time point of step
186 detection definition, a further analysis was performed: Time periods where activPAL3™ outcomes
187 were within ± 4 steps (i.e. ± 2 strides – one for the start and one for the end of the time segment)
188 were identified. The proportion of walks within ± 4 steps was examined against speed and cadence.
189 This analysis allowed for a difference in interpretation of the number of steps taken between the
190 video observation and activPAL3™. This might have arisen due to a difference in the exact point of a
191 step being detected/counted between the video observation and the activPAL3™. Such differences
192 would simply have been due to the definitions used in the analysis and not necessarily true
193 differences in outcomes. This method of data analysis, therefore, provides insight into 'definite'
194 discrepancies between outcomes of the video observation and activPAL3™.

195 As one monitor was used on each thigh and as the monitors output is based on strides detected the
196 outcomes of the two monitors were compared. To provide an overview of outcomes, results are

197 presented using all outcomes from both right and left activPAL3™ together as examples of possible
198 outcomes arising from the monitor.

199 Normality of outcomes was tested (Shapiro-Wilk test). The outcomes of the monitors across the
200 range of speeds were compared using the Wilcoxon Signed Rank Test and the correlation tested
201 using paired sample correlations.

202

203 **Results**

204 All twenty participants (age 36±10;20:54 years, (mean ± standard deviation; minimum: maximum),
205 height 172±9;154:189 cm, weight 68±10;55:87 kg) completed all parts of the testing protocol giving
206 800 walking periods with 80 at each walking speed.

207 Distributions of outcomes at lower speeds were not normal, therefore, for consistency, all data is
208 presented as median with interquartile range. Both cadence (Figure 1) and step length calculated
209 from video observation reduced with reduction in speed of walking. Across the range from 0.1 to
210 1.0 m/s the best fit second order polynomials between speed (m/s), cadence (steps/min) and step
211 length (m) were:

212 Cadence (steps/min) = $-47.727 \times [\text{Speed (m/s)}]^2 + 132.23 \times [\text{Speed (m/s)}] + 13$ ($R^2 = 0.9963$)

213 Step length (m) = $-0.1741 \times [\text{Speed (m/s)}]^2 + 0.5795 \times [\text{Speed (m/s)}] + 0.1998$ ($R^2 = 0.9975$)

214

215  Insert figure 1 here

216

217 The proportion of walks with intermittent stepping was higher at lower speeds and cadences (Figure
218 2). Only 11% of walks were continuous at 0.1m/s, whilst all were continuous at and above 0.4m/s.

219 In general below 40 steps/min walking was predominantly intermittent. However, there were
220 examples of intermittent stepping at up to 100 steps/min. Intermittent stepping predominantly
221 occurred at low cadences and relatively high step length. Combinations of cadence and step length
222 appeared to fall into two patterns with a set of combinations not used by participants (Figure 2).

223

224  Insert figure 2 here

225

226 The outcomes from the two monitors (left and right legs) were not identical (% steps across speeds;
227 related samples Wilcoxon Signed Rank Test, $p=0.008$), but the overall outcomes demonstrated
228 similar trends (paired sample correlations, 0.870). Therefore to provide an overview of activPAL3™
229 performance the following results are derived from the outcomes of the activPAL3™ on the right leg
230 and that on the left leg combined.

231 The percentage of steps detected dropped from 95.2% at 0.6m/s to 0% at 0.1m/s (Figure 3A). There
232 was rapid reduction in % steps detected below 0.5m/s. With cadence (Figure 3B) there was a similar
233 trend for reduced % step detection with reduction in cadence. Below 69 steps/min (% steps
234 detected 95.6%) the step detection became erratic (large interquartile range), again reducing to 0%
235 step detection at 24 steps/min.

236

237 Insert figures 3A and 3B here

238

239 The percentage of trials within ± 4 steps of that determined from video observation was over 90% at
240 and above 0.6m/s (Figure 4A). However, there was a marked reduction at 0.5m/s (67%), with
241 smaller proportions of trials within ± 4 steps below this speed, reducing to 17% at 0.2m/s. When
242 examined by cadence of stepping all trials above 75 steps/min had over 90% of trials within ± 4 steps
243 (Figure 4B). There was a steep reduction in % of trials within ± 4 steps below this cadence reaching
244 approximately 30% at a cadence of 50 steps/min.

245

246 Insert figures 4A and 4B here

247

248 **Discussion**

249 The characterisation of stepping activity provides insight into physical activity performance and can
250 be used to provide objective evidence of engagement in free-living everyday activity. Establishing
251 the validity of activity monitors across the range of outcome measures reported is important to
252 ensure correct interpretation of outcomes. Stepping activity at low stepping rates (cadences) has
253 been reported in the literature for the activPAL™ [6], yet there is limited evidence of the validity of
254 these outcomes for either the activPAL™ or the activity monitor examined in this work, the
255 activPAL3™. Not only is it important to understand if the monitor can detect slow stepping, but it is
256 also important to understand if the reported stepping activity is actually continuous or might be
257 constituted of intermittent stepping portrayed as continuous very slow cadence stepping.

258 There is emerging evidence that the activPAL™ monitor does not have a high level of validity at low
259 speeds of walking [13-15]. Whilst examination of monitor validity by walking speed is useful, the
260 monitor actually outputs cadence. Very low cadence has been reported [6] without evidence of the
261 validity of these measurements. If the monitor does not reliably detect stepping below a certain
262 cadence threshold it is likely that any stepping reported below this threshold is actually intermittent
263 stepping interpreted by the monitor signal analysis algorithms as continuous stepping. This may be
264 individual or very short bouts of relatively high cadence stepping joined together with intervening
265 standing events to appear as very low cadence stepping.

266 The outcomes of this study indicate that there is a relatively consistent relationship between
267 apparent speed of progression, mean step length and mean cadence across the speed range studied
268 with excellent fit to a quadratic best fit line (Figure 1).

269 Participants were asked to walk in a self-selected manner at the prescribed treadmill speeds. There
270 was considerable variation in the way that the participants walked at the slower speeds, with some
271 choosing to use an intermittent pattern of walking. This was particularly prevalent below a speed of

272 0.4m/s and a cadence of 45 steps/min (Figure 2). The variation in stepping pattern is emphasised by
273 the range of combinations of cadence and step length that were chosen at each speed of stepping
274 (Figure 2). There appeared to be combinations of cadence and step length that were not used,
275 perhaps indicating that these were the least physiologically appropriate combinations for efficiency
276 of movement. However, some participants chose to use high cadence and short step length
277 combinations at the lower speeds distinct from the majority of participants who used lower cadence
278 and longer step length.

279 The results are presented by cadence and speed calculated across each 20s period, however, for
280 intermittent walking there would have been periods where stepping did not occur. Some individuals
281 were able to walk continuously at 0.1m/s, although it would appear that a speed of 0.2m/s might be
282 considered the minimum continuous walking speed for the majority of the participants.

283 The % of steps detected is used here as a means of characterising the validity of the activPAL3™s.
284 The results demonstrate that the activPAL3™s were capable of determining stepping activity well
285 (>90% median step detection) at and above 0.5m/s (Figure 3A) and 69 steps/min (Figure 3B). Below
286 this level the ability of the monitor to detect steps declined rapidly. The speed threshold of 0.5m/s
287 is in agreement with activPAL™ outcomes previously reported by Taraldsen et al [13], Kanoun [14]
288 and Lutzner et al [15] who identified weaker performance below this level: Taraldsen below
289 0.47m/s, Kanoun at 0.45m/s and Lutzner below 0.6m/s. It should be noted that the equivalence of
290 outcomes between the activPAL™ and activPAL3™ has not been demonstrated. The addition of
291 information on the decrease in step detection with cadence provides evidence of a validity threshold
292 that can be directly related to the results generated by the activPAL3™, as the activPAL3™ does not
293 characterise speed of walking, only cadence.

294 Whilst the examination of the results by % steps detected provides insight into performance, the
295 protocol used provided challenges with data interpretation that could result in overestimation of
296 errors. Within each 20s period there would have been differences in video vs. activPAL3™

297 interpretation at the start and end of the period. The exact point of stride detection by the
298 activPAL3™ was not known and may not be the point of foot contact as used in this study.
299 Therefore, it is possible that an extra stride may have been detected or one missed by the
300 activPAL3™ at the start and end of each period of stepping compared to those counted by video
301 analysis. By examining the results based on all trials within ± 4 steps, absolute errors in step
302 detection could be identified (Figures 4A and 4B). This analysis revealed that performance dropped
303 below 90% of trials within this range at and below 0.5m/s or 75 steps/min. This indicates that there
304 were definite missed steps below these thresholds. This type of end effect error would have an
305 impact on any examination of the validity using a fixed time period analysis. If stepping had been
306 observed over longer time periods then this apparent error would have still been present, but its
307 overall percentage impact on outcomes would have been smaller. However, there was a close
308 relationship between the thresholds below which performance deteriorated for % steps and trials
309 within ± 4 steps. This agreement provides reassurance that the thresholds are true representations
310 of monitor validity.

311 The activPAL3™ outputs steps and the time at which these occur. Therefore, its main output is
312 instantaneous cadence. When steps were missed by the activPAL3™ this was sometimes classified
313 as upright standing with no stepping, but in other cases consecutive steps were lumped together as
314 one with an allocated very low cadence. The misclassification of output of the activPAL3™, as seen
315 by the user, might therefore be either stepping activity classed as quiet standing or artificially low
316 cadence stepping. It was not possible to determine a consistent pattern of how stepping at low
317 speeds/cadences would be characterised by the activPAL3™.

318 The outcomes of this study, indicating a low or reduced percentage of steps detected for slower
319 speeds, are similar to those found for other step detection devices. For example, Cyarto et al [16]
320 report for the Yamax Digiwalker (DW-200) that for nursing home residents that from 0.80 ± 0.35 m/s
321 down to 0.42 ± 0.17 m/s the percentage error in step count increased from 46.3 ± 38.1 to 73.9 ± 34.8 %.

322 However, in contrast there are reports for other monitors that slow stepping can be detected:
323 Macko et al [17] report that it is possible using the SAM monitor to gain high levels of accuracy at
324 low cadences, achieving an accuracy of $98.5 \pm 1.0\%$ for step detection at cadences of 46 ± 8.9
325 steps/min in stroke patients. Therefore, with the right combination of technology and data analysis
326 methods it is clearly possible to detect stepping at very slow speeds.

327

328 Limitations

329 The participants were a convenience sample of healthy adults, without pathology. It is not possible
330 to say how these results would apply to other groups, especially those with movement pattern
331 disorders.

332 These results are based on treadmill stepping activity. It is possible that stepping activity performed
333 over-ground may be performed differently to that on a treadmill at very low speeds.

334 The activPAL3™ did not have any real time output and it was, therefore, not possible to
335 automatically synchronise its output with that of the video recorder. This meant that
336 synchronisation had to be accomplished manually by identifying matching points in the data
337 streams. The approach taken was to use walking at 1.0m/s as the reference within the activPAL3™
338 s. This method explicitly assumed that the activPAL3™ s were recording the first stride of walking at
339 1.0m/s. Inspection of the results confirmed this assumption. However, it is possible that the
340 synchronisation was out by up to the time of one stride. This fact contributed to the need to use
341 only the middle 20s of each 30s walking block within the walking cycles. Whilst longer walking
342 blocks may have been desirable, this duration was used to reduce overall burden on participants
343 whilst allowing repetition of the walking cycles. It would be beneficial for future protocols to extend
344 recording time of constant speed stepping to reduce the significance of end effect errors. However,

345 this must take into account the limits of participant performance to reduce the chance of fatigue
346 affecting results.

347

348 **Conclusion**

349 Participants were likely to use an intermittent stepping pattern below 0.4m/s or a cadence of 45
350 steps/min. The activPAL3™ detects over 90% of steps taken at and above a walking speed of 0.5m/s
351 and a cadence at and above 69 steps/min. Below these thresholds the monitor detects decreasing
352 numbers of steps with no steps detected at 0.1m/s and at or below 24 steps/min.

353 When using the activPAL3™ to determine outcomes of stepping activity, cadence reported below 69
354 steps per minute should be interpreted cautiously. Similarly when stepping activity below 0.5m/s is
355 anticipated careful consideration of outcome validity should be made to reduce the possibility of
356 misinterpretation of outcomes.

357 **Acknowledgements**

358 The authors would like to thank all volunteers for their participation.

359 This work was performed as part of study at Glasgow Caledonian University with no external
360 funding.

361 Ethical approval given by Glasgow Caledonian University School of Health and Life Sciences Ethics
362 Committee (Ref: HLS12/108).

363

364 **References**

- 365 1. World Health Organization (2010) Global Recommendations on Physical Activity for Health.
366 ISBN 978 92 4 159 997 9.
- 367 2. Garber CE, Blissmer B, Deschenes MR, Franklin BA, Lamonte MJ, Lee IM, et al. American
368 College of Sports Medicine position stand. Quantity and quality of exercise for developing
369 and maintaining cardiorespiratory, musculoskeletal, and neuromotor fitness in apparently
370 healthy adults: guidance for prescribing exercise. *Med Sci Sports Exerc.* 2011;43:1334–59.
- 371 3. Bohannon RW. Comfortable and maximum walking speed of adults aged 20-79 years:
372 reference values and determinants. *Age and Ageing* 1997;26:15-19.
- 373 4. Peel NM, Kuys SS, Klein K. Gait speed as a measure in geriatric assessment in clinical settings:
374 A systematic review. *J Gerontol A Biol Sci Med* 2012;68:39-46.
- 375 5. Studenski S, Perera S, Patel K, Forano C, Faulkner K, Inzitari M, Brach J, Chandler J, Cawthon
376 P, Barrett Connor E, Nevitt M, Visser M, Kritchevsky S, Badinelli S, Harris T Newman AB,
377 Cauley J, Ferrucci L, Guralnik J. Gait speed and survival in older adults. *J A M A* 2011;305:50-
378 58.
- 379 6. Dall PM, McCrorie PRW, Granat MH, Stansfield BW. Step accumulation per minute epoch is
380 not the same as cadence for free-living adults. *Med Sci Sports Exerc.* 2013;45:1995-2001.

- 381 7. Aminian S & Hinckson EA. Examining the validity of the ActivPAL monitor in measuring
382 posture and ambulatory movement in children. *Int J of Behavioural Nutrition and Physical*
383 *Activity* 2012; 9:119:2-9.
- 384 8. Harrington DM, Welk GJ, Donnelly AE. Validation of MET estimates and step measurement
385 using the ActivPAL physical activity logger. *J of Sports Sciences* 2011;29:627-633.
- 386 9. Dahlgren G, Carlsson D, Moorhead A, Hager0Ross C, McDonough SM. Test-retest reliability
387 of step count with the ActivPAL™ device in common daily activities. *Gait & Posture*
388 2010;32:386-390.
- 389 10. Maddocks M, Petrou A, Skipper L, Wilcock A. Validity of three accelerometers during
390 treadmill walking and motor vehicle travel. *British Journal of Sports Medicine* 2010;44:606-
391 608.
- 392 11. Ryan CG, Grant PM, Tigbe WW, Granat MH. The validity and reliability of a novel activity
393 monitor as a measure of walking. *British Journal of Sports Medicine* 2006;40:779-784.
- 394 12. Grant PM, Dall PM, Mitchell SL, Granat MH. Activity-monitor accuracy in measuring step
395 number and cadence in community-dwelling older adults. *Journal of Aging and Physical*
396 *Activity* 2008;16:201-214.
- 397 13. Taraldsen K, Askim T, Sletvold O, Einarsen E, Bjastad KG, Indredavik B, Helbostad J.
398 Evaluation of a body-worn sensor system to measure physical activity in older people with
399 impaired function. *Physical Therapy* 2011; 91:277-285.
- 400 14. Kanoun N. Validation of the ActivPAL activity monitor as a measure of walking at pre-
401 determined slow walking speeds in a healthy population in a controlled setting. *Reinvention:*
402 *a Journal of Undergraduate Research* 2009;2.
403 <http://www.warwick.ac.uk/go/reinventionjournal/issues/volume2issue2/kanoun>
404 [20/01/2014].

- 405 15. Lutzner C, Voigt H, Roeder I, Kirschner S, Lutzner J. Placement makes a difference: Accuracy
406 of an accelerometer in measuring step number and stair climbing. *Gait & Posture*
407 2014;1126-1132.
- 408 16. Cyarto EV, Myers AM, Tudor-Locke C. Pedometer accuracy in nursing home and community-
409 dwelling older adults. *Med Sci Sports Exerc* 2004;36:205-209.
- 410 17. Macko RF, Haeuber E, Shaughnessy M, Coleman D, Boone DA, Smith GV, Silver KH.
411 Microprocessor-based ambulatory activity monitoring in stroke patients. *Med Sci Sports*
412 *Exerc* 2002;34:394-399.
- 413
- 414

415 **Table legends**

416 Table 1

417 Treadmill protocol including a warm up, 4 stepping cycles (see text for description of cycles A and B)
418 and rest breaks.

419

420 **Figure legends**

421 Figure 1

422 Relationship between video derived cadence and treadmill speed. Median and interquartile range
423 of all results at each speed. The best fit second order polynomial line is overlaid.

424 Figure 2

425 The combination of mean cadence and mean step length used to achieve stepping speed and the
426 occurrence of continuous (closed circles) and intermittent stepping (open circles). All trials of all
427 participants are included. The distinct rows of outcomes are related to speed of treadmill walking as
428 indicated (m/s).

429 Figure 3

430 Percentage of steps detected by A) treadmill speed and B) video cadence (median and interquartile
431 range).

432 Figure 4

433 Percentage of activPAL3TM outputs within +/- 4 steps of video steps by A) treadmill speed and B)
434 video cadence (median and interquartile range).

Figure 1

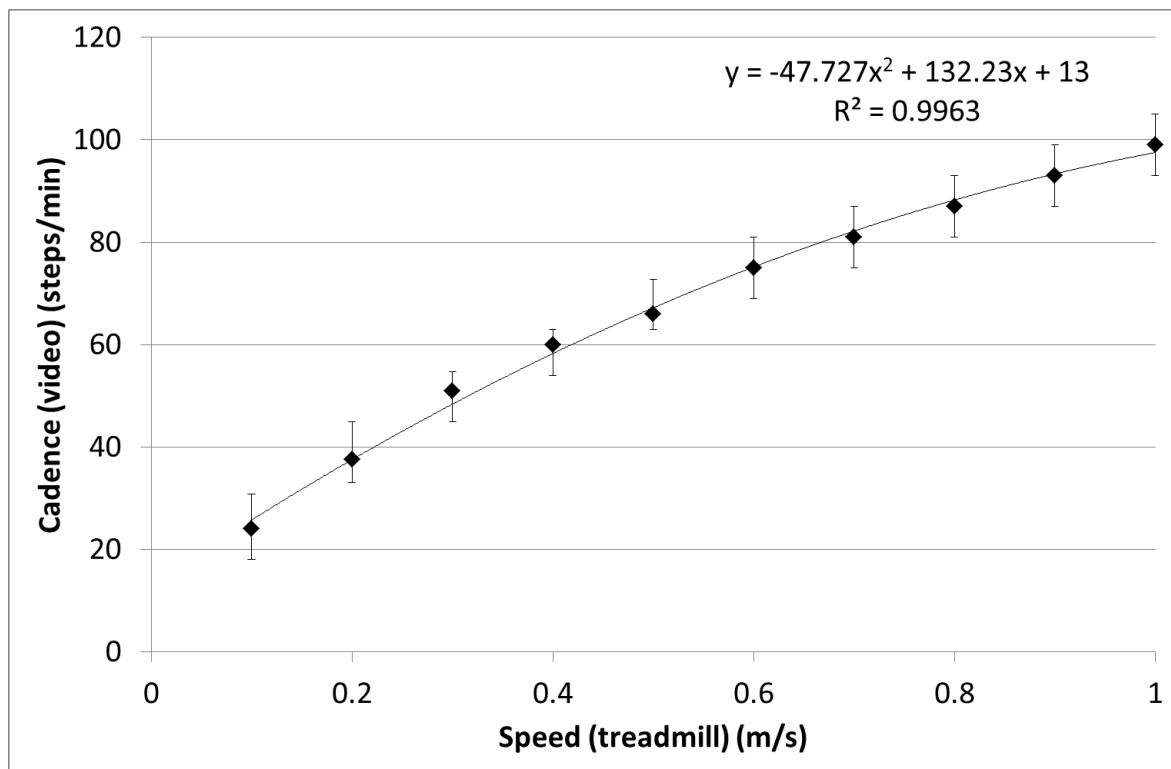


Figure 2

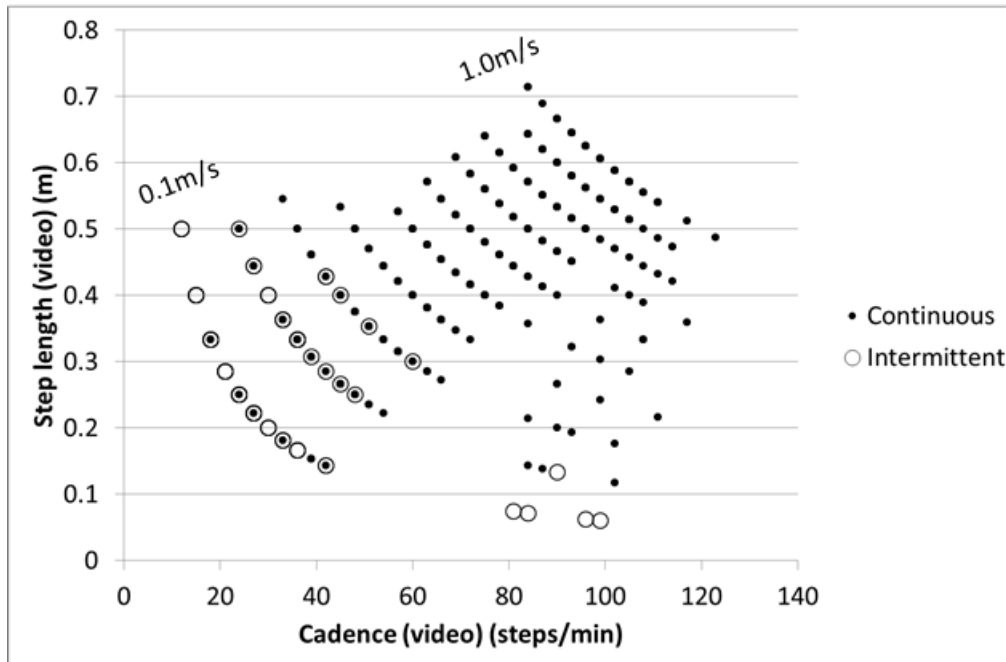
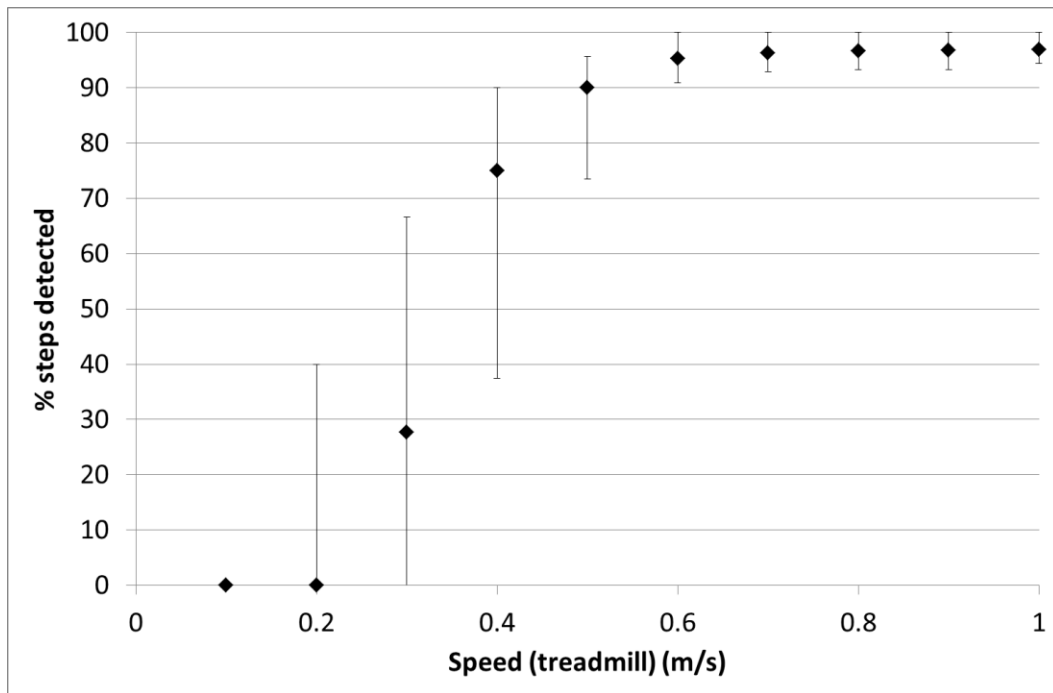


Figure 3A



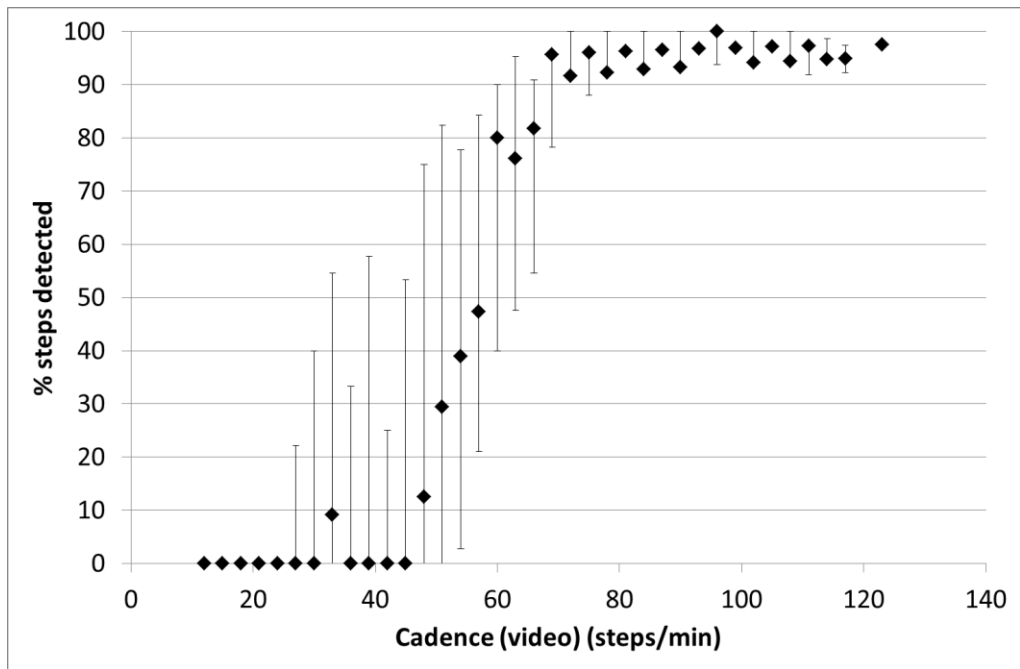


Figure 4A

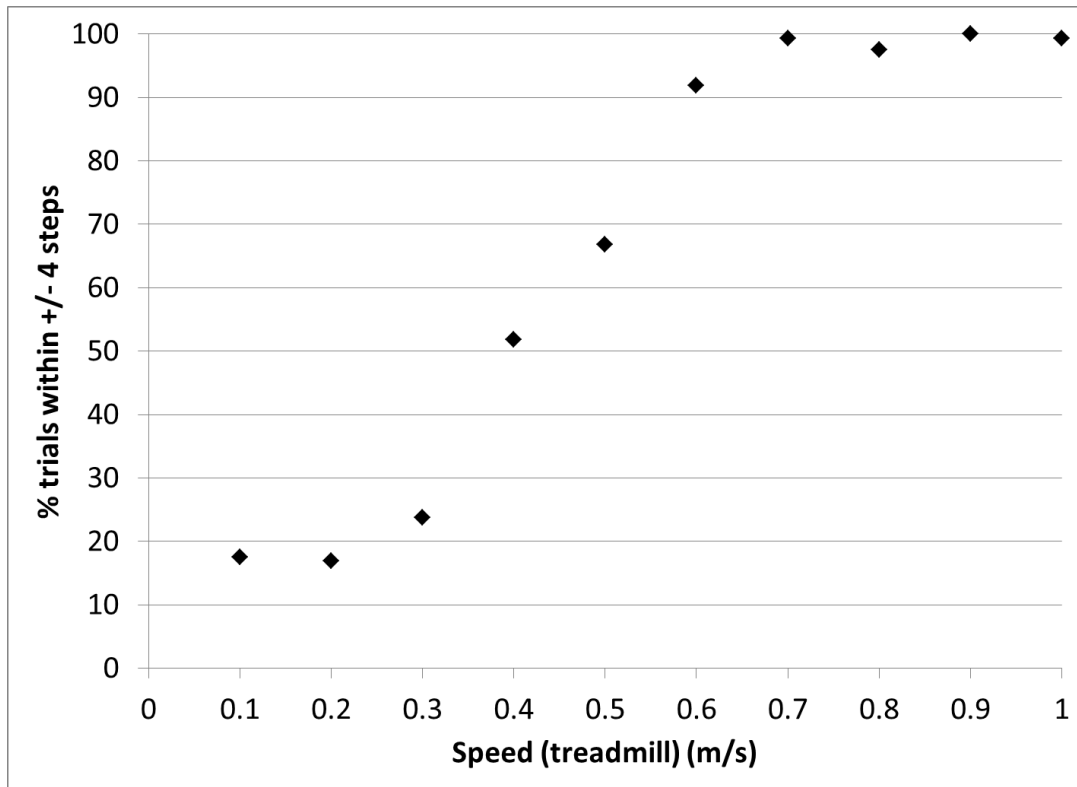


Figure 4B

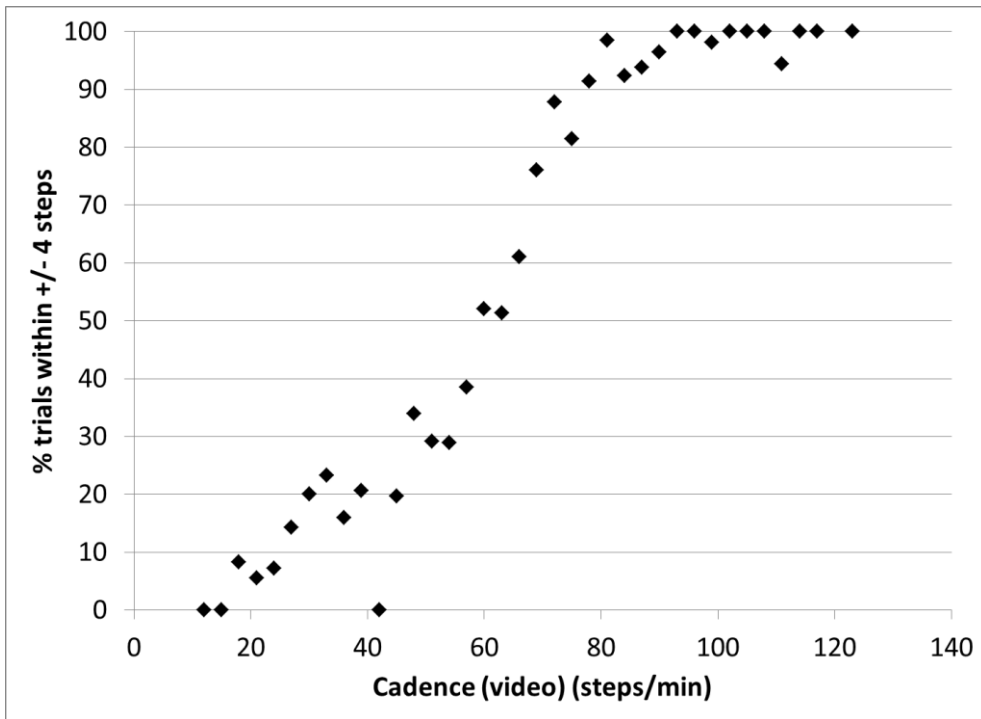


Table 1 Treadmill protocol including a warm up, 4 stepping cycles and rest breaks. There were two stepping cycles, A and B:

A (Descending cycle) = decreasing from 1.0 m/s to 0.10 m/s, in 0.1m/s decrements each 30 seconds

B (Ascending cycle) = increasing from 0.10m/s to 1.0m/s, in 0.1m/s increments each 30 seconds

Treadmill protocol	Action	Duration
Warm up	Stepping, 0.1m/s to 1.0m/s	2 mins
rest	Standing on the treadmill	1 min
Stepping cycle 1	Stepping, either cycle A or B	5 mins
rest	Standing on the treadmill	1 min
Stepping cycle 2	Stepping, either cycle A or B	5 mins
rest	Standing on the treadmill	2 min
Stepping cycle 3	Stepping, either cycle A or B	5 mins
rest	Standing on the treadmill	1 min
Stepping cycle 4	Stepping, either cycle A or B	5 mins
rest	Standing on the treadmill	1 min